the LCD and the current displayed value will be frozen. To return from the held reading, press the button again.

Max/Min: Press and hold the Max/Min button for at least 3 seconds until "MAX" icon appears on the LCD to view the current Max reading. To view the current Min reading, press the button again and the "MIN" icon will appear. To exit the Max/Min mode, press and hold the Max/Min button for 3 seconds.

The meter will conduct measurement and select measurement range automatically.

The measuring level range is from 30dB to 130dB.

Hold the meter in hand or use a tripod to affix the meter in the desired location. The best measuring distance is 1 to 1.5m away from the sound source to the microphone.

8. Operation Precautions

- 1) Do not store or operate the meter in areas of high temperature or humidity.
- 2) Remove the battery when the meter is to be stored for long periods of time to avoid battery leakage.
- 3) Wind blowing across the microphone will affect the noise measurement. Use the supplied wind muffler to cover the microphone during applications involving turbulent air.
- 4) Keep microphone dry and avoid severe vibration.

9. Calibration

Repairs, servicing and calibration should only be performed by York Survey Supply Centre. The recommended calibration period is 1 year.



Prospect House, George Cayley Drive, Clifton Moor, York, England YO30 4XE

Tel: +44 (0) 1904 692723 Fax: +44 (0) 1904 690385 E-Mail: sales@yorksurvey.co.uk www.yorksurvey.co.uk



Mini Sound Level Meter



Operating Instructions

Ref:.. \operat98\instructions 15\343090.qxp 05-01-15

Mini Sound Level Meter

User Manual

Please read this user manual thoroughly before using this unit and keep it for your future reference.

1. Safety

Read the following safety information carefully before attempting to operate the meter. Use the meter only as specified in this manual; otherwise, the warranty may be invalidated.

- Environment Conditions:
- Altitude up to 2000 metres
- RH<90% (Non-condensation)
- Operating temperature: -20 ~ 60°C
- Maintenance:
- Repairs or servicing should only be performed by York Survey Supply Centre.
- Wipe the unit with a dry soft cloth. Do not use abrasives or solvents on this instrument. Complies with EMC.

2. Introduction


This sound level meter is designed to meet the measurement requirements of safety engineers, health, industrial safety offices and sound quality control in various environments like factories, schools, construction sites, etc.

- · Complies with IEC61672-1 Class 2 standard
- · "A" frequency rating
- Data hold
- Max/Min measured values

3. Specifications

Applied standard	IEC61672-1 Class 2	Max hold	MAX
Accuracy	±1.4dB	Min hold	MIN
Frequency range	31.5Hz to 8,000Hz	Data hold	HOLD
Measuring range	30dB to 130dB	Display	3½ digits
Frequency weighting	dBA	Battery life	at least 30 hours
Dynamic range	50dB	Operating conditions	-20°C to 60°C 10%RH to 90%RH
Microphone	½" electret condenser	Storage conditions	-20°C to 60°C 10%RH to 75%RH
Auto power off	After approx 15 minutes of inactivity	Power supply	1x 9V PP3 alkaline battery
Resolution	0.1dB	Dimensions (LxWxH)	144 x 55 x 38mm
Sample rate	0.5 sec	Weight	90g

4. Meter Description

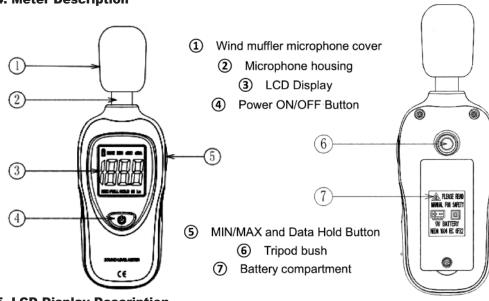

5. LCD Display Description



ICON	FUNCTION	
LCD	3½ digits	
MAX	Max value hold	
MIN	Min value hold	
dBA	"A" frequency weighting (designed to reflect the response of the human ear to noise)	
HOLD	Data hold	
	Low battery indication	

6. Basic Operation

- a) Open the battery cover and install a 9 volt battery in the battery compartment.
- b) Close the battery compartment
- c) When the low battery icon appears, replace the battery.

7. Operation Instructions

1) Backlight & Power On/Off Function

Power On: To turn the meter on, press the power button for 1 second until the LCD is lit, then release the button.

Power Off: To turn the meter off, press and hold the power button for approx. 3 seconds until the LCD switches off, then release the button.

Backlight: After turning the meter on, momentarily press the power button and the backlight will turn on/off. It will automatically turn off after approx. 30 seconds of inactivity.

2) Data Hold & Max/Min Function

Hold: After turning the meter on , momentarily press the Max/Min button, "HOLD" will appear on

Ref:.. \operat98\instructions 15\343090.qxp 05-01-15